Typical Carbon X/XL Installation

FUJIFILM

Carbon X/XL

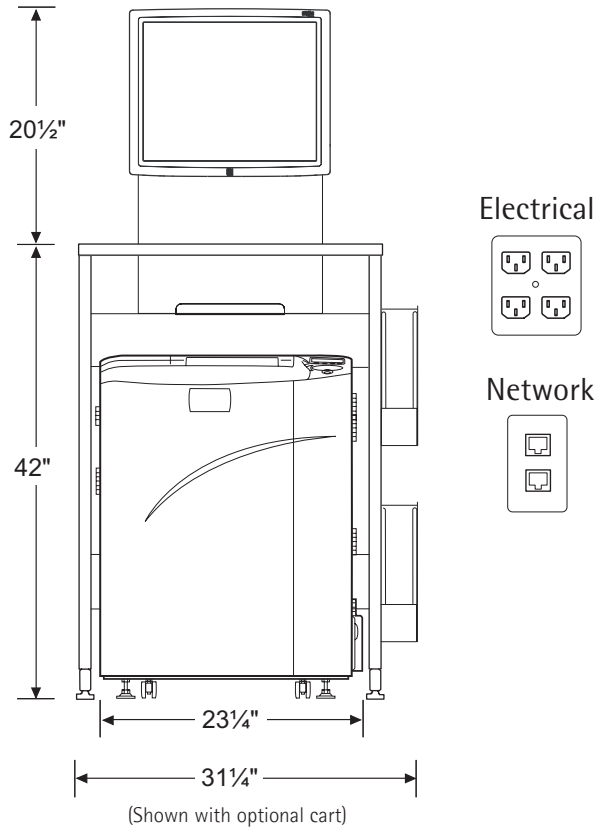

(Shown with optional cart)

Electrical Requirements:

* Quad 110 volt outlet (20 amp dedicated line)

  Reading Unit: 110 volts, 5 Amps
  CPU: 110 volts, 2 Amps
  LCD Display: 110 volts, 0.6 Amps

* 2 Network Drops
  RJ-45 connections. 100 base-T network
  Network switch setting:
  #1 Full Duplex, #2 ½ Duplex

Physical Specifications:

* 39¼" Minimum space during operation
  (includes 8" space on either side)

  Total weight: 216 lbs
  Overall Height: 32"
  Width: 23¼"
  Depth: 15"

Note: Dimensions and weight refer only to the Carbon Reader and does not include the optional cart or the Flash IIP Workstation.

Environmental Conditions:

Temperature range: 59-86 degrees Fahrenheit
Humidity Range: 40-80% RH
Heat Output: 995 BTU/hour or lower

* *Minimum requirements*

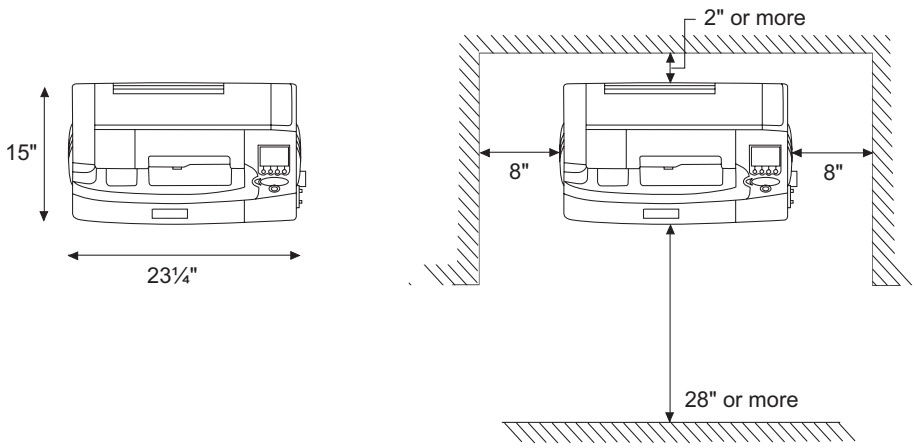

FUJIFILM Medical Systems USA, Inc.
www.fujimed.com

Corporate Headquarters
419 West Avenue
Stamford, CT 06902-6300
203-324-2000
800-431-1850

CSS-0007870-A 01/12/2006